


PAC CHECK® Model 325

Hand-held O₂ & CO₂ Headspace Analyzers



DURABLE

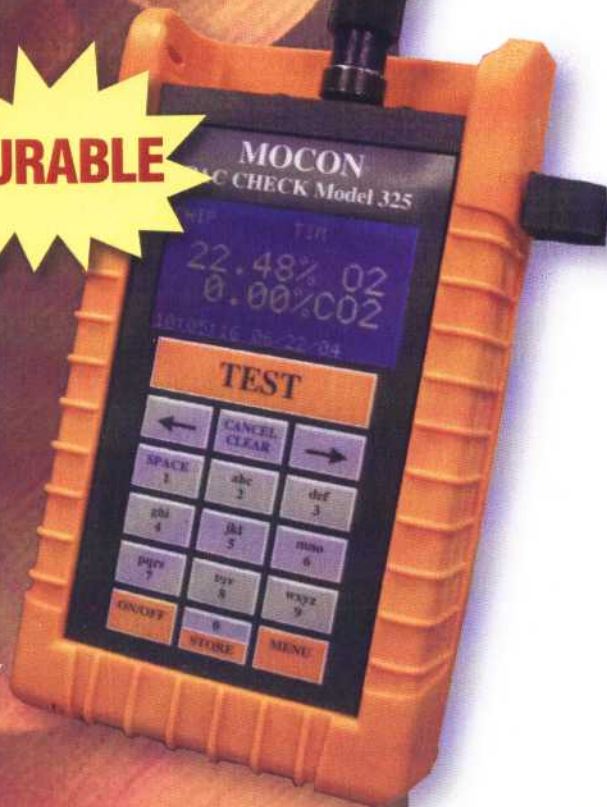

NEW TECHNOLOGY



- Portable
- Fast
- Accurate results
- Easy-to-use & Read

Hand-held measurement of O₂/CO₂ concentration in packages

The PAC CHECK® Model 325 is a single-handed Oxygen and Carbon Dioxide analyzer for checking modified atmospheres inside packages. It is the ideal instrument for portable, fast and accurate headspace tests on the packaging line, in warehouses or in laboratories.

You can be certain that QA/QC checks are being performed since this analyzer has the ability to store 400 readings, sorted by operator and product name. The PAC CHECK Model 325 is the ideal instrument for sample tests with only a minimum gas required for even the smallest packs in a Modified Atmosphere Package.

Benefits

- Safe to use. Our optional Sticky FootSM probe assembly shields the needle for your protection and has a built-in long-lasting septum. No need to apply a new septum for every package!
- Test small packages. The PAC CHECK Model 325 has the ability to test packages with a minimum sample size of less than 4 ml (3 ml in manual mode).
- Test more packages quicker. With a response time within 7 seconds; this analyzer is fast.
- Long-lasting batteries for a full day's work. You can take 2,000 samples on one full charge and with the Auto off feature, you will preserve the life of your charge.
- Easy to use anywhere. This analyzer is portable and can be used anywhere with one hand or as a bench top with the easel back feature.
- Rugged protective boot (including security strap) helps to prevent damage when dropped and is easy to clean.
- Simple and accurate 1, 2, or 3-point calibration.

mocon®

Typical applications where portability would be effective.

- All Modified Atmosphere Packaging
- Meat/Poultry
- Coffee
- Cheese
- Nuts
- Snack Food Packaging
- Bakery
- Pet Foods
- Pharmaceuticals
- Oxygen Scavenger Performance
- Beverages

Specifications

Accuracy - O ₂ Sensor	±0.1% abs or 2% rel whichever is greater
Range - O ₂ Sensor	Oxygen – 0 to 100%
Response	98% of final value within 7 seconds
Resolution (O ₂ or CO ₂)	0.01%
Oxygen Measurement Method	Chemical Cell
Carbon Dioxide Measurement Method	Infrared
Range of CO ₂ Sensor	0 - 100%
Accuracy of CO ₂ Sensor	2% abs @ 0 - 20%; 3% abs @ 20 -100%
Calibration (O ₂ or CO ₂)	1, 2 or 3-point calibration
Sample Method	Auto internal sampling pump. (Manual Injection optional)
Adjustable Pump Time	1 - 9 sec.
Barometric Pressure Range	400 - 760 mmHg
Memory	400 data points stored
Display	128 x 68 LCD
Dimensions & Weight	7.5" x 4.3" x 2.3" 1.7 lbs. (with batteries and protective boot)
Ambient Operating Temperature	0 - 40 C (0 to 45 C storage)
Ambient Humidity	10 to 90% non-condensing
Minimum Sample Size	<4 cc auto – (3 cc with manual option)
Supply Voltage	100 -240 VAC or 4,2000 mah NiMH rechargeable batteries
Supply Frequency	50/60 Hz (includes battery recharger)
Languages	English, Spanish, Italian, German and French
Markings	CE, CSA, and UL

mocon®

7500 Boone Ave. North
Minneapolis, MN 55428
USA
763-493-6370
www.mocon.com

Table Top Use



PAC CHECK Series to fit all your Bench top, Hand-held, O₂, CO₂ and Combination O₂ & CO₂ testing needs.

Date	Time	Partial
10/20/00	10:00:00	0.100000
10/20/00	10:01:00	0.100000
10/20/00	10:02:00	0.100000
10/20/00	10:03:00	0.100000
10/20/00	10:04:00	0.100000
10/20/00	10:05:00	0.100000
10/20/00	10:06:00	0.100000
10/20/00	10:07:00	0.100000
10/20/00	10:08:00	0.100000
10/20/00	10:09:00	0.100000
10/20/00	10:10:00	0.100000
10/20/00	10:11:00	0.100000
10/20/00	10:12:00	0.100000
10/20/00	10:13:00	0.100000
10/20/00	10:14:00	0.100000
10/20/00	10:15:00	0.100000
10/20/00	10:16:00	0.100000
10/20/00	10:17:00	0.100000
10/20/00	10:18:00	0.100000
10/20/00	10:19:00	0.100000
10/20/00	10:20:00	0.100000

Data Grab™ Software Option
Software is available to organize and save the data from the Model 325.

For complete specifications for your application, please call.

MOCON and PAC CHECK are registered trademarks, and
DATA GRAB is trademark of MOCON.
PC325/704

Made in USA